

# Operating instructions

## RVO/U-L2 Module BASICS

### Flow Monitor



Series RVO/U-L2

Type RVO/U-L20012 thru RVO/U-L20500

Read this manual prior to performing any task!

Meister Strömungstechnik GmbH

Im Gewerbegebiet 2

63831 Wiesen

Germany

Telephone: +49 6096 9720 - 0

Fax: +49 6096 9720 - 30

E-mail: [sales@meister-flow.com](mailto:sales@meister-flow.com)

Internet: [www.meister-flow.com](http://www.meister-flow.com)

RVO/U-L2 Modul BASICS, 2, en\_US

These instructions were compiled by:

Meister Strömungstechnik GmbH

Subject to change without notice

© Meister Strömungstechnik GmbH 2021

These instructions facilitate the safe and efficient handling of a flow monitor (referred to as "device" in the following). The instructions are an integral part of the device and must be kept within easy reach for the personnel in the immediate vicinity of the device at all times. Personnel must carefully read and understand these instructions before commencing all work. The basic requirement for safe work is adherence to all safety and handling instructions stipulated in these instructions. The local accident-prevention regulations and general safety standards and regulations for the field of application of the device also apply. Illustrations in these instructions are provided to aid general understanding and might deviate from the actual model. No claims can be derived from any such differences.

### **Limitations of liability**

All details and instructions in this manual have been compiled under consideration of the valid standards and regulations, the current state-of-technology and our many years of knowledge and experience. The manufacturer does not accept any liability arising from:

- non-observance of any details in these instructions
- improper use of the device, or use that is not in accordance with these instructions
- use of non-trained personnel

- unauthorized retrofitting or technical changes that have not been authorized by the manufacturer
- use of non-approved replacement parts

The duties and obligations agreed upon in the delivery contract apply in full, as well as the general terms and conditions, the terms of delivery by the manufacturer and the valid legal regulations applicable at the conclusion of the contract.

### **Copyright**

These operating instructions are protected by copyright.

Except for internal purposes, transfer of these instructions to third-parties, copying them in any way – even in part – as well as dissemination and/or communication of their content is forbidden without prior written authorization from Meister Strömungstechnik ("manufacturer"). Violations are subject to claims for indemnification. The manufacturer reserves the right to assert additional claims.

Copyright is the property of the manufacturer.

© Meister Strömungstechnik GmbH

Im Gewerbegebiet 2

63831 Wiesen

Germany

# Table of contents

<b>1</b>	<b>Overview</b>	<b>7</b>
1.1	Short description	7
1.2	Warranty and guarantee provisions	7
1.3	Customer service	7
<b>2</b>	<b>Safety</b>	<b>8</b>
2.1	Explanation of symbols	8
2.2	Correct use in accordance with these instructions	10
2.3	Special precautions	11
2.3.1	Hazards from electrical current	12
2.3.2	Mechanical hazards	12
2.3.3	Hazards from high or low temperatures	13
2.3.4	Radiation hazards	14
2.3.5	Hazards caused by media	14
2.4	Personnel requirements	15
2.5	Personal safety equipment	15
2.6	Protective systems	16
2.7	Replacement parts	17
2.8	Environmental protection	17
2.9	Responsibility of the owner	18
<b>3</b>	<b>Design and function</b>	<b>20</b>
3.1	Overview	20
3.2	Device description	20
3.3	Component description	21
<b>4</b>	<b>Transport, packaging and storage</b>	<b>22</b>
4.1	Safety instructions for transport	22
4.2	Transport inspection	22
4.3	Packaging	22
4.4	Symbols on the shipping box	23
4.5	Storage	23
<b>5</b>	<b>Installation and initial startup</b>	<b>25</b>
5.1	Safety	25

5.2	Requirements at the place of installation.....	25
5.3	Preparatory work.....	26
5.4	Installation in the pipe system.....	30
5.5	Initial startup.....	33
5.6	Electrical connection.....	34
5.6.1	Switch contact SG-15 with connector in compliance with EN 175301-803.....	35
5.6.2	Switch contact SG-15 with plug connector M12x1.....	36
5.6.3	Switch contact SG-15 with cable.....	37
5.6.4	Degree of protection (IP-Code).....	37
5.7	Grounding the device.....	37
5.8	Plug connection.....	38
5.9	Contact protection measures.....	40
<b>6</b>	<b>Operation.....</b>	<b>42</b>
6.1	Setting the switch point.....	42
6.2	Checking the flow.....	44
<b>7</b>	<b>Troubleshooting.....</b>	<b>46</b>
7.1	Safety.....	46
7.2	Troubleshooting guide.....	48
<b>8</b>	<b>Maintenance.....</b>	<b>50</b>
8.1	Safety.....	50
8.2	Maintenance plan.....	50
8.3	Removal from the pipe system.....	51
8.4	Disassembly.....	53
8.5	Maintenance.....	56
8.5.1	Cleaning.....	56
8.5.2	Parts replacement.....	57
8.5.3	Assembly.....	57
8.5.4	Switch contact replacement.....	64
8.6	Measures to be taken after maintenance work.....	66
<b>9</b>	<b>Disassembly and disposal.....</b>	<b>67</b>
9.1	Safety.....	67
9.2	Disassembly.....	67

9.3	Return Materials.....	67
9.3.1	Return Materials Authorization.....	67
9.4	Disposal.....	68
<b>10</b>	<b>Technical data.....</b>	<b>69</b>
10.1	Device data plate.....	69
10.2	Switch contact rating plate.....	69
10.3	Dimension sheet.....	70
10.4	General specifications.....	71
10.5	Electrical specifications.....	72
10.6	Measuring ranges.....	74
10.6.1	Standard measuring ranges.....	74
10.7	Operating data.....	75
<b>11</b>	<b>Annex.....</b>	<b>76</b>
11.1	Tightening torque.....	76
11.2	Replacement parts.....	77
11.3	Tools.....	78
11.4	Sealant.....	78
11.5	Lubricants.....	79
<b>12</b>	<b>Index.....</b>	<b>80</b>

# 1 Overview

## 1.1 Short description

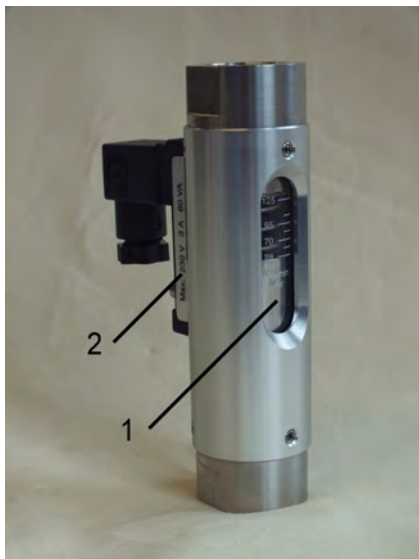


Fig. 1: RVO/U-L2 flow monitor

- 1 Sight glass with measuring scale
- 2 Switch contact with female socket or connecting cable

The flow monitor RVO/U-L2 monitors the continuous flow of gaseous media. It is designed for installation in pipe systems.

A float inside the device is moved by the medium flowing through it. The current rate of flow can be read-off on the measuring scale on the sight glass. The top edge of the float is the read-off point.

External measuring devices can be connected at the socket.

## 1.2 Warranty and guarantee provisions

Warranty and guarantee provisions are contained in the general terms and conditions of Meister Strömungstechnik.

## 1.3 Customer service

For technical support, please contact our customer service department (for contact details, see Page 2).

Furthermore, our staff is always interested in receiving new information and experiences gained from application of the device, which may be useful in improving our products.

## 2 Safety

This chapter provides an overview of important safety aspects required for optimum protection of personnel as well as for safe installation and safe operation of the device.

Non-observance of the handling and safety instructions listed in this manual may result in hazardous/dangerous conditions and in damage to property.

### 2.1 Explanation of symbols

#### Safety instructions

Safety instructions in this manual are marked by symbols. The safety instructions are preceded by signal words that indicate the level of danger/hazard.

To prevent accidents or injury to persons as well as damage to property, always observe the safety instructions and proceed carefully.



#### **DANGER!**

This combination of symbol and signal word indicates an immediate, dangerous condition that results in death or serious injury if it is not avoided.



#### **WARNING!**

This combination of symbol and signal word indicates a possibly dangerous condition that might result in death or serious injury if it is not avoided.





### CAUTION!

This combination of symbol and signal word indicates a possibly dangerous condition that might result in minor or slight injury if it is not avoided.



### NOTICE!

This combination of symbol and signal word indicates a possibly dangerous condition that might result in damage to property and to the environment if it is not avoided.



Designates step-by-step handling instructions



Designates a state or an automatic sequence as a result of a specific operating step



Designates randomly ordered enumerations and list entries



“Signs used in these instructions” on page 9, designates references to chapters in these instructions

## Tips and recommendations



*This symbol emphasizes useful tips and recommendations as well as information for efficient and failure-free operation.*

## Signs used in these instructions

The following signs and highlightings are used in these instructions to identify handling instructions, the description of results, lists/enumerations, references and other elements:

## 2.2 Correct use in accordance with these instructions

The device has been designed and constructed solely for the correct use in accordance with these instructions.

*Table 1: Correct use in non-hazard areas*

The flow monitor serves exclusively to monitor the continuous flow of gaseous media within a temperature range of -20 °C to 100 °C (optional: 160 °C) at a maximum operating pressure of 16 bar.

### Correct use in explosion-hazard zones

For employment in explosion-hazard zones, changed conditions apply for the intended use.

The intended use in explosion-hazard zones is described in the Operating Instructions "RVO/U-L2 Module ATEX".

Intended use in explosion-hazard zones includes the observance of all specifications in these Operating Instructions, as well as those for "RVO/U-L2 Module ATEX".

Any additional or different application, above or beyond the correct use in accordance with these instructions, is deemed as incorrect use.



### WARNING!

#### Danger due to incorrect use!

Incorrect use of the flow monitor may result in dangerous conditions.

- Use the flow monitor only within the stipulated performance limits
- Do not subject the flow monitor to severe temperature fluctuations
- Do not use the flow monitor with quick-acting valves
- Do not use the flow monitor with solenoid valves
- Do not subject the flow monitor to vibrations
- Do not subject the flow monitor to pressure surges
- Do not use the flow monitor with media containing solids or abrasives
- Only use the flow monitor with media previously approved by the manufacturer
- Do not use the flow monitor as the sole monitoring device to prevent dangerous conditions
- Do not install the flow monitor as a load bearing part within a pipeline system

- The flow monitor with sight glass must be installed in such a way as to preclude damage to the sight glass by outside force. If necessary, install an appropriate impact protection device

All claims for damages due to incorrect usage are excluded.

## 2.3 Special precautions

The following section lists residual risks that might arise from the device.

To reduce health risks and prevent dangerous situations, observe the safety instructions listed here as well as the safety instructions in the other chapters of these operating instructions.



### **DANGER!**

**Employment of the device in explosion-hazard zones requires the observance of the Operating Instructions for "RVO/U-L2 Module ATEX" including all hazard statements and warnings, therein.**



*These operating instructions cannot cover all conceivable dangers because many dangers arise, not from the device itself, but from the respective media flowing through it. Always observe the appropriate safety data sheets when using hazardous media!*

## 2.3.1 Hazards from electrical current

### Electrical current



#### **DANGER!**

#### **Danger to life from electrical current!**

There is an immediate risk to life from electrocution on touching live parts. Damaged electrical insulation or components can be extremely dangerous.

- Only qualified electricians shall work on the electrical system.
- If the insulation is damaged, immediately switch off and have repairs performed.
- Before commencing work on live parts of the electrical systems and operating equipment, disconnect the equipment and ensure that it remains disconnected for the duration of the work. Observe these 5 safety rules when doing so:
  - Isolate (disconnect)
  - Secure against switching back on
  - Check for absence of voltage
  - Ground and short

- Cover or cordon off other live parts in the vicinity
- Never bridge fuses or put them out of operation. Always observe the correct current ratings when replacing fuses
- Keep moisture away from live parts. This can result in short-circuit

## 2.3.2 Mechanical hazards



#### **WARNING!**

#### **Risk of injury from glass breakage!**

The sight glass in the flow monitor can burst due to excessive temperature or pressure. There is a risk of injury from glass splinters and escaping media.

- Keep within the stipulated operating limits
- Wear personal protective equipment
- Avoid severe temperature fluctuations
- Avoid pressure surges



**WARNING!**

**Risk of injury on sharp edges and pointed corners!**

Sharp edges and pointed corners can cause abrasions and skin cuts.

- Proceed with caution when working near sharp edges and pointed corners.
- If in doubt, wear protective gloves.

## 2.3.3 Hazards from high or low temperatures

### Hot or cold surfaces



**WARNING!**

**Risk of injury from hot or cold surfaces!**

Surfaces of components may heat up/cool down dramatically due to the media flowing through them. Skin contact with hot or cold surfaces may cause severe skin burn or frostbite.

- Always wear temperature-resistant protective work clothing and protective gloves when working near hot/cold surfaces
- Before commencing work, make sure that all surfaces have been cooled down or warmed up to ambient temperature

## 2.3.4 Radiation hazards

### Strong magnetic fields



#### **WARNING!**

#### **Danger to life from strong magnetic fields!**

Strong magnetic fields may cause severe injury or even be fatal, as well as cause considerable damage to property.

- Persons with pacemakers must not be located in the vicinity of the device. This could impair the function of the pacemaker
- Persons with metal implants must not be located in the vicinity of the device. Implants can heat up or be attracted magnetically
- Keep ferromagnetic materials and electromagnets away from the magnetic source. These materials could be attracted and fly through the room, thereby injuring or even killing persons. Minimum clearance: 3 m
- Remove and put away metal objects before maintenance work (jewelry, watches, writing implements, etc.)

- Do not place any electronic devices within the vicinity of the magnetic source. These could be damaged
- Do not place any electronic storage media, credit cards, etc. within the vicinity of the magnetic source. Data could be deleted

## 2.3.5 Hazards caused by media

### Hazardous media



#### **WARNING!**

#### **Risk of injury from hazardous media!**

If the flow monitor is used for toxic, corrosive or very hot/cold media, there is a risk of serious injury from escaping media.

- Observe details in the safety data sheet of the media
- Comply with the safety, accident prevention and environmental protection regulations appropriate to the media used
- Wear personal protective equipment in accordance with the safety data sheet

## 2.4 Personnel requirements



### **WARNING!**

#### **Risk of injury due to insufficiently trained and qualified personnel!**

If unqualified personnel work on the device or are located within its hazard zone, dangers arise which may result in serious injury and considerable damage to property.

- All work must be performed by qualified personnel only.
- Keep unqualified personnel away from hazard zones.

Authorized personnel is to be restricted to those persons who can be expected to perform their work reliably. Persons whose ability to respond is influenced, e.g. by drugs, alcohol or medication, are not authorized.

Observe the age and occupational regulations at the site when choosing personnel.

The following lists the personnel qualifications for the various areas of activity:

### **Qualified electrician**

Due to specialized training, knowledge and experience as well as knowledge of the relevant standards and regulations, the qualified electrician is able to independently perform work on the electrical systems as well as to detect and avoid possible risks and dangers.

Additionally, the electrician must provide proof of his/her professional qualification that certifies his/her ability to perform work on electrical systems.

The qualified electrician must fulfill the requirements contained in the valid legal accident-prevention regulations.

### **Qualified personnel**

Due to their specialized training, knowledge and experience as well as their knowledge of the relevant standards and regulations, qualified personnel are able to independently perform the work assigned to them as well as to detect and avoid possible risks and dangers.

## 2.5 Personal safety equipment

Personal safety equipment is used to protect personnel from hazards/dangers that might impair their safety or health during work.

When performing the various tasks at, and with the device, personnel must wear personal safety equipment. Special reference is made of this in the individual chapters within these Operating Instructions. The following provides a description of the personal safety equipment:

- Always wear appropriate personal safety equipment required in the various chapters of these Operating Instructions before commencing work.
- Comply with the personal safety equipment instructions posted within the work area.

## Description of personal safety equipment

**As specified in the Safety Data Sheet of the medium, protective equipment must be worn when handling hazardous media. In addition, the specifications of the system operator must be followed. If no protective equipment is specified, suitable protective gloves and goggles must be worn.**

The protective equipment is used to protect against hazardous media leaks and hazardous media residue in the device.

## Goggles



The goggles are used to protect the eyes from flying debris and splashing fluid.

## Protective gloves



Protective gloves protect the hands from friction, burns, grazing, abrasion, surface cuts or deeper injuries, as well as from direct contact with hot or cold surfaces.

## 2.6 Protective systems

### Integration within an emergency-stop concept is required

The device is designed for use as a part of a machine or system. It does not have its own controller and does not have an autonomous emergency-stop function.

Before starting up the device, install the emergency-stop equipment and incorporate it into the safety chain of the machine or system.

Connect the emergency-stop equipment so that if there is an interruption in the power supply or in the activation of the power supply after an interruption, dangerous conditions are excluded for persons and valuables.

The emergency-stop equipment must always be freely accessible.



## 2.7 Replacement parts



### **WARNING!**

#### **Risk of injury due to use of incorrect replacement parts!**

Use of incorrect or faulty replacement parts may result in dangers to personnel as well as damages, malfunctions or total failure.

- Only use original replacement parts from the manufacturer or approved by the manufacturer.
- Always contact the manufacturer in case of doubt.

Always purchase replacement parts from an authorized dealer or directly from the manufacturer (For contact details, see Page 2).

The replacement parts list is in the annex.

## 2.8 Environmental protection



### **NOTICE!**

#### **Risk to the environment due to improper handling of environmentally hazardous substances!**

Serious environmental damage may result if substances harmful to the environment are handled incorrectly, especially if they are disposed of improperly.

- Always observe the instructions listed below on the handling and disposal of substances harmful to the environment.
- If harmful substances are released into the environment, take immediate countermeasures. If there is doubt, contact the local authorities, inform them of the damage and request information on suitable countermeasures to be taken.

### **Cleaning fluids**

Solvent-based cleaning fluids contain toxic substances. They must never be released into the environment and must be disposed of by a waste management company.

## Lubricants

Lubricants such as greases and oils contain toxic substances. They must never be released into the environment and must be disposed of by a waste management company.

## 2.9 Responsibility of the owner

### Owner

The owner is the person who operates the device himself for business or commercial purposes or who cedes such use/application to a third-party and who, during operation of the device, has full legal product stewardship for protection of the user, the personnel or third-parties.

### Duties of the owner

The device is used in the commercial sector. The owner of the device is therefore subject to legal obligations pertaining to work safety.

In addition to the safety instructions contained in these Operating Instructions, the safety, accident prevention and environmental protection regulations applicable to the field of application of the device must be observed.

In particular, this includes:

- The owner must inform himself regarding the valid health and safety regulations and must perform a risk assessment to additionally determine the risks resulting from the special work

conditions arising at the location at which the device is used, especially in regard to the media used. He must then implement these within Operating Instructions for use of the device.

- **For the USA:**

The "Occupational Health and Safety Act" of 1970 stipulates that it is the duty of the owner to provide a safe workplace. He must hereby ensure that the device is operated and maintained compliant to valid commercial, industrial, local, federal and state laws, standards and regulations.

- **For Canada:**

The "Canadian Centre for Occupational Health and Safety Act" of 1978 stipulates that all Canadians have "...a fundamental right to a healthy and safe working environment." It is therefore the duty of the owner to provide a safe workplace. He must ensure that the device is operated and maintained compliant to valid commercial, industrial, local, provincial, territorial and federal laws, standards and regulations.

- Appropriate to the working conditions and the media used, the owner must affix signs within the working area that inform the user of the hazards and dangers present.

- During the entire period of use of the device, the owner must check periodically to ensure that the Operating Instructions correspond to the current state of regulations, and he must make adjustments as necessary.
- The owner must clearly regulate and determine responsibilities for installation, operation, troubleshooting, maintenance and cleaning.
- The owner must fit/retrofit suitable safety equipment within the complete plant/system.
- The owner must ensure that all staff/personnel have thoroughly read and understand these instructions before handling the device. Additionally, he must train the personnel at regular intervals and warn them of dangers.
- The owner must provide the personnel with the required safety equipment and must instruct them that its wear is mandatory.
- The owner must ensure that the maintenance intervals described in these Operating Instructions are adhered to at all times.
- The owner must ensure that the device is completely free of all residual media before disposal. Remains of corrosive or toxic materials must be neutralized.

Additionally, the owner is responsible for ensuring that the device is always kept in a technically perfect condition. The following therefore applies:

- The owner must implement suitable safety measures, appropriate to the media used.
- Different media have different severities of influence on the soiling and wear of/to the device. The owner must set suitable maintenance intervals, depending on the media flowing through the device.

## 3 Design and function

### 3.1 Overview

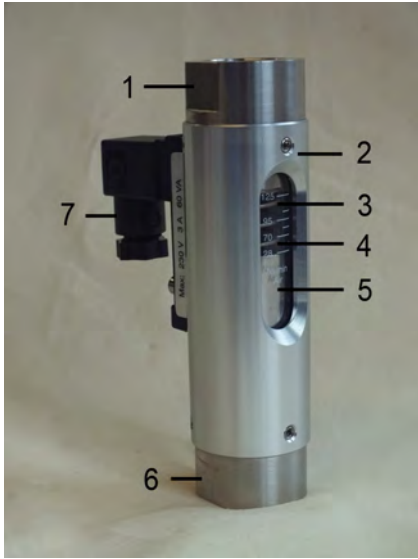


Fig. 2: Front view

- 1 Process connection (outlet)
- 2 Device body
- 3 Spring
- 4 Sight glass with measuring scale
- 5 Float
- 6 Process connection (inlet)
- 7 Switch contact and female socket  
or switch contact with cable

### 3.2 Device description

RVO/U-L2 flow monitors operate on the principle of the variable area flow-meter. The flow monitor is installed into a pipe system and measures the flow rate of the medium flowing through the pipe system.

A float inside the flow monitor is moved by the flowing medium. A magnetic field is generated by the magnets inside the float. The position of the float is detected by the switch contact. In addition to electrical control by the Reed-contact (switch contact), the current flow can also be read-off on the measuring scale on the sight glass.

Applications for RVO/U-L2 flow monitors are, for example, supply circuits transporting gaseous media. The device monitors the volume flow of the supply medium to ensure proper operation. If the flow drops below the threshold preset by the operator, the switch contact (change-over contact) switches or opens (normally open contact).

### 3.3 Component description

#### Switch contact



*Fig. 3: Switch contact and female socket*

A potential-free Reed-contact is cast into the switch contact housing assembly (Fig. 3/1). The device is supplied with a connector (Fig. 3/2).

#### Sight glass



*Fig. 4: Sight glass*

A measuring scale is burnt onto the sight glass, from which the current rate of flow can be read-off.

## 4 Transport, packaging and storage

### 4.1 Safety instructions for transport

#### Improper transport

#### NOTICE!

**The device could be damaged if transported improperly!**

Objects to be transported may fall or overturn if transported improperly. This may result in damage to the device and/or property.

- Proceed carefully when unloading transported packages, both on delivery and when transporting in-house. Observe the symbols and instructions on the shipping box
- Remove packaging material just prior to assembly

### 4.2 Transport inspection

On delivery, make an immediate check for completeness and check for transport damages.

If there are any visible external transport damages, proceed as follows:

- Do not accept the delivery
- Note the damage in the shipping documents or on the delivery note of the transporter and have the driver confirm by signature
- Initiate a claim for damages



*Make a claim for each fault as soon as it is detected. Claims for damages can only be invoked within the valid claim periods.*

### 4.3 Packaging

#### About packaging

The packaging serves to protect the individual components from transport damages, corrosion and other damages until they are installed. Do not discard the packaging and only remove the device from the shipping box immediately before installation.

## Handling packaging materials

Dispose of packaging material in accordance with the valid legal regulations and local ordinances.

### **! NOTICE!**

#### **Danger to the environment due to incorrect disposal!**

Packaging is made of valuable raw materials and can be reused in many cases or usefully processed and recycled. Improper disposal of packaging materials may pose a danger to the environment.

- Dispose of packaging material in an environmentally safe manner
- Comply with the local disposal regulations. If necessary, have the packaging disposed of by approved specialists.

## 4.4 Symbols on the shipping box

### Top



The arrows indicate the top side of the package. They must always point upwards, otherwise the content may be damaged.

## Fragile



Designates packages with breakable or damageable contents.

Handle the package carefully and do not allow it to fall or be subjected to jarring or severe vibration.

## 4.5 Storage

### Storing the packages

Store the packages under the following conditions:

- Do not store in the open
- Store dry and dust-free
- Do not subject to any aggressive media
- Protect from direct sunlight
- Avoid mechanical vibrations and shocks
- Storage temperature: 0 to 35 °C / 32 °F to 95 °F
- Relative humidity: max. 60 %
- Do not stack
- If storing for longer than 3 months, regularly check the general condition of all parts as well as of the packaging.



*Storage instructions in addition  
to the instructions listed here  
may be listed on the packages.  
Follow these instructions also.*



## 5 Installation and initial startup

### 5.1 Safety

#### Incorrect installation and initial startup



#### **WARNING!**

#### **Risk of injury due to incorrect installation and initial startup!**

Incorrect installation and initial startup may result in severe injury and considerable damage to property.

- Ensure that the site is sufficiently cleared of obstructions before commencing work
- Handle open or sharp edged components carefully
- Ensure that the assembly location is orderly and clean! Parts and tools lying about or on top of each other are potential causes for accidents
- Assemble components properly. Observe the stipulated tightening torque of screws
- Before initial startup, make sure that all installation work has been performed and completed in compliance with the specifications and instructions in these Operating Instructions

#### Safeguard against restart



#### **WARNING!**

#### **Danger to life due to unauthorized restart!**

There is a risk of severe or even fatal injury due to unauthorized restart of the power supply during installation.

- Before commencing work, switch off the power supply to the entire system/plant and secure against restart

### 5.2 Requirements at the place of installation

The place of installation must meet the following requirements:

- The device must not be under water.
- The surrounding area must be sufficiently illuminated.
- There must be sufficient space to prevent accumulation of trapped heat.
- The device must not be installed as a supporting part in a pipe construction.
- The device may not have anything affixed to, or suspended from it.

- The flow monitor must be installed in such a way as to preclude damage by outside force. It must be ensured that the flow monitor cannot be damaged. If necessary, install an appropriate impact protection device.
- External magnetic fields will influence the switch contact. Keep sufficient distance to magnetic fields (e.g. electric motors).
- Piping, process connections or supports made of ferromagnetic material influence the magnetic field of the device. Keep a space of minimum 100 mm to those materials (e.g. steel).

## 5.3 Preparatory work

The following criteria must be met during installation to ensure correct functioning of the flow monitor:




### WARNING!

#### **Danger due to incorrect installation!**

If the criteria listed above are not observed when installing the flow monitor, dangerous/hazardous conditions may arise.

- Do not install the flow monitor as a supporting part in a pipe system
- Do not use the flow monitor with quick-acting valves
- Do not use the flow monitor with solenoid valves

### Installation position/direction of flow

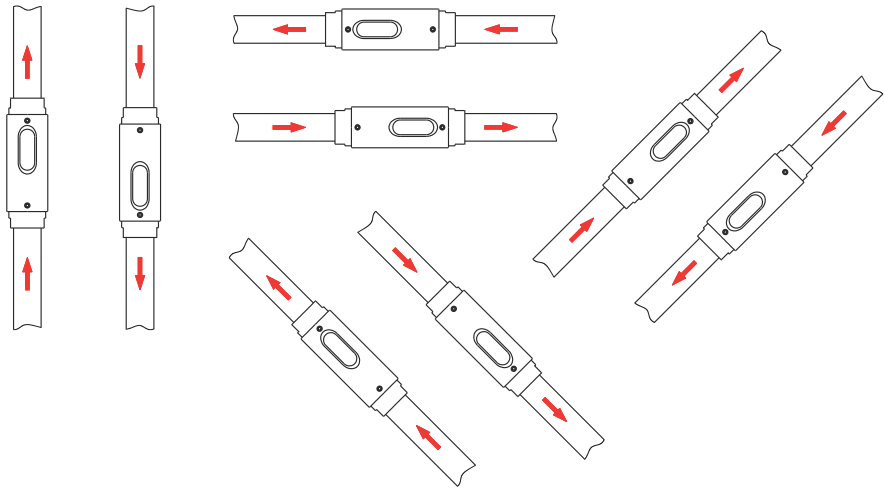

*Fig. 5: Installation position/direction of flow*

The flow monitor must only be installed in one of the positions displayed above. The medium must flow in the direction of the arrow (from a low to a high scale value).

## Unimpeded flow sections


**! NOTICE!****Measuring inaccuracy due to incorrect installation!**

The measuring accuracy of the flow monitor is influenced by its position within the pipe system. Changes in cross-section, branch-offs or bends in the pipe system impair measuring accuracy.

- Ensure that the unimpeded flow sections are maintained
- Never reduce the pipe diameter immediately before the device



*We recommend unimpeded flow sections, type BS-228.*

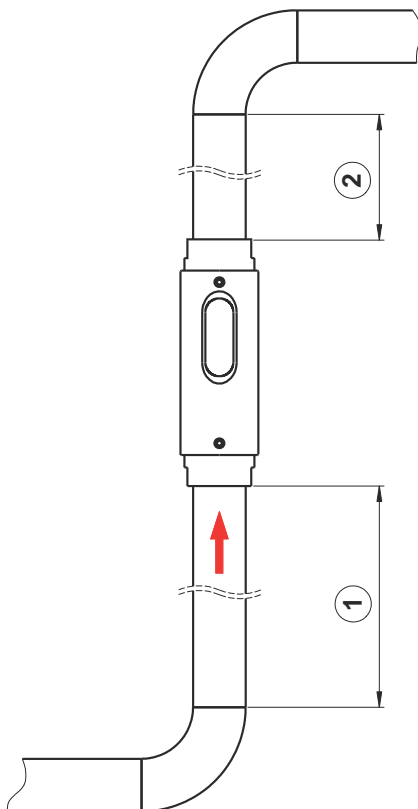

**Fig. 6: Unimpeded flow section**


- 1 10 x DN
- 2 5 x DN

- There must be an unimpeded flow section of 10 x DN (rated width) before the device.
- There must be an unimpeded flow section of 5 x DN (rated width) after the device.

### Unimpeded outlet

If the pipe system ends at an unimpeded outlet, the flow monitor must not be installed directly in front of the opening.

### Strainer

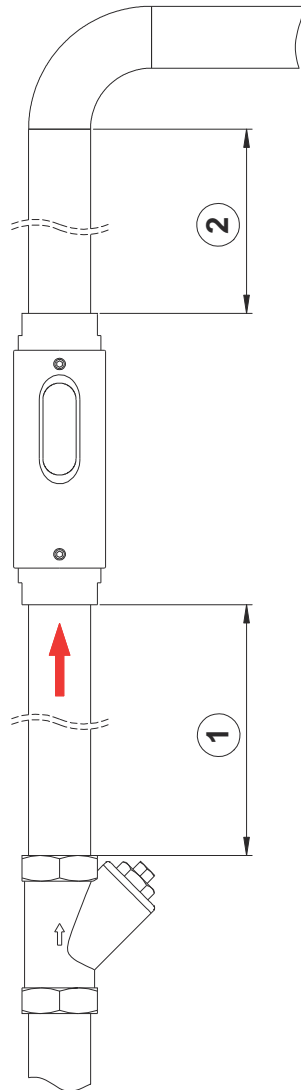

*Fig. 7: Strainer*

- 1 min. 10 x DN
- 2 min. 5 x DN

If the medium is contaminated by solids, a strainer must be installed before the device (Fig. 7).



*We recommend a Type SF, SFD or SFM.*



### Prepare the device

#### NOTICE!

##### **Risk of damage to property due to contamination!**

Contamination and deposits may impair the free movement of the float, thereby damaging the device.

- Ensure that there are no foreign particles in the device
- Ensure that the device is not soiled
- Do not use any media containing solids

-  1. Remove the device from the shipping carton and visually inspect the device to ensure that it is free of packaging materials.
-  2. Check device for soiling and clean, if necessary.

## 5.4 Installation in the pipe system



#### **WARNING!**

##### **Risk of injury from pressurized lines!**

If the pipe system is under pressure when installing the device, severe injuries may result.

- Depressurize the pipe system before installing the device



## WARNING!

### Risk of injury from hot or cold surfaces!

Pipelines can heat up/cool down dramatically due to the media flowing through them. Skin contact with hot or cold surfaces may cause severe skin burn/freezing.

- Before commencing work, ensure that the system has been controlled to a temperature range between 0 and 40 °C.
- Do not touch any parts of the system that are either very cold or very hot.
- Always wear heat-resistant/cold-resistant protective work clothing and protective gloves when working near hot/cold surfaces



## WARNING!

### Risk of injury from media in the pipe system!

If the pipe system contains toxic or other hazardous media, severe injuries may be caused by escaping media.

- Before installation, ensure that the pipe system is empty and does not contain any media residue
- Always wear personal protective equipment during installation
- Provide suitable draining devices (collection tank, etc.)



## NOTICE!

### Risk of damage to device due to contaminated pipe system!

Dirt and foreign particles entering the device can damage the device and impair its operation.

- Ensure that the pipe system is clean before installing the device.
- If necessary, flush the pipe system with clean medium before installation




*A suitable sealant must be selected, depending on the condition/composition of the pipe lines, the medium and the operating and environmental conditions. The sealing method described here is only an example and cannot be used in all cases.*

### Sealing the pipe connection

#### Personnel:

- Qualified personnel

#### 1. → Nap the thread.

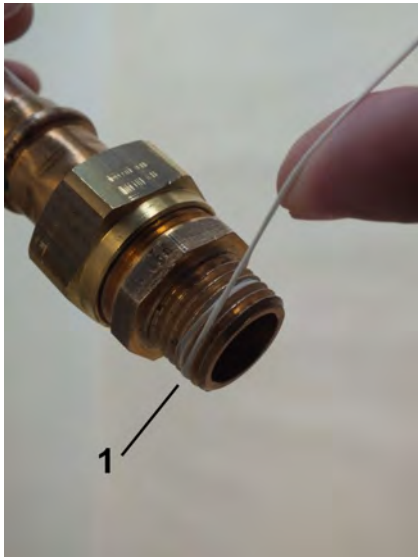

**Fig. 8: Apply sealing thread**

2. → Apply sealing thread (Fig. 8/1) to the napped area in the threaded direction. Observe the quantity recommended by the sealant manufacturer.



**Fig. 9: Pipe connection with sealing thread**

- ⇒ The pipeline is now ready for assembly (Fig. 9)



### Install device in pipe system

#### Personnel:

- Qualified personnel

#### Protective equipment:

- Protective gloves

#### Tool:

- Fixed spanner



#### CAUTION!

Do not hold the device by its threads. These are sharp edged and may cause injury.

1. ➤ Place the threaded end of the device onto the thread of the connecting pipe



Fig. 10: Screw in the device

2. ➤ Fasten the adapter union of the pipeline with an appropriate spanner (Fig. 10/1). When doing so, lock the process connection of the device in place to prevent slip, using a suitable spanner (Fig. 10/2).



Fig. 11: Screw in the device

3. ➤ Keep turning in the adapter union (Fig. 11/1) while holding the process connection of the device locked (Fig. 11/2) until the connection is tight
4. ➤ Repeat these steps at the other end of the device.

## 5.5 Initial startup

The following steps must be taken before initial startup and any subsequent startup (e.g. after removal and installation during maintenance).

1. **WARNING!**

Make sure that the plant is operating vibration-free. Vibrations could destroy the device. This could result in a serious risk of injury to the user.

2. **WARNING!**

Make sure that the medium is flowing continuously. Pulse-like staggered loads could destroy the device. This could result in a serious risk of injury to the user.

3. **NOTICE!**

Flush the pipe system carefully and ensure that there are no solids or other foreign matter in the system. These could impair the function, or even damage the device.

## 5.6 Electrical connection

The electrical connection of the flow monitor is accomplished through the connector plug or the cast on power cable leading from the switch housing. The switch contacts employed in these devices are potential free and do not require a power source. Switch contacts and flow monitor have been optimally harmonized. After replacement of a switch contact, the switch point must be readjusted.

**DANGER!****Danger to life from electrical current**

There is an immediate risk to life from electrocution on touching live parts. Damage to the electrical insulation or single components can be extremely dangerous.

- Only qualified electricians shall work on the electrical system
- If the insulation is damaged, immediately switch off and have repairs performed.

- Before commencing work on live parts of electrical systems and components, disconnect the equipment and ensure that it remains disconnected for the duration of the work. Observe these 5 safety rules when doing so:
  - Isolate (disconnect)
  - Secure against switching back on
  - Check for absence of voltage
  - Ground and short
  - Cover or cordon off other live parts in the vicinity
- Never bridge fuses or put them out of operation. Always observe the correct current ratings when replacing fuses
- Keep moisture away from live parts. This may result in short-circuit

### 5.6.1 Switch contact SG-15 with connector in compliance with EN 175301-803

Wiring diagram of the supplied socket (EN 175301-803, Form C) front view.

Wiring diagram

Normally Open (NOC):

#### EN 175301-803



Fig. 12: Switch position under no-flow condition

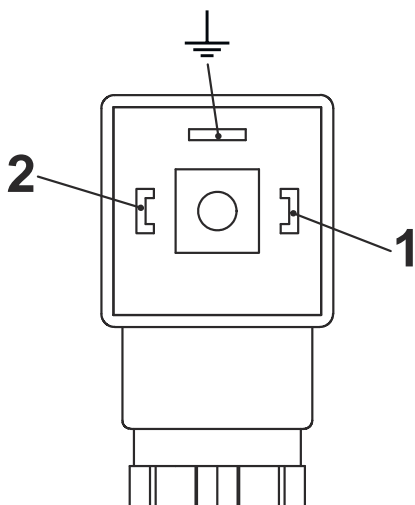


Fig. 13: Pin assignment, plug socket, normally open contact. The ground-pin is not used.

Change Over (COC):

#### EN 175301-803



Fig. 14: Switch position under no-flow condition

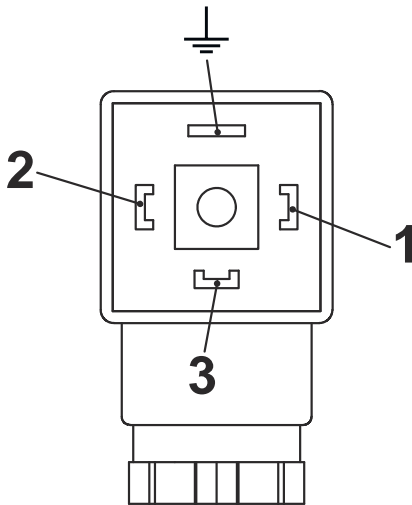


Fig. 15: Pin assignment, plug socket, change over contact. The ground-pin is not used.

### 5.6.2 Switch contact SG-15 with plug connector M12x1

Wiring diagram, connector M12x1

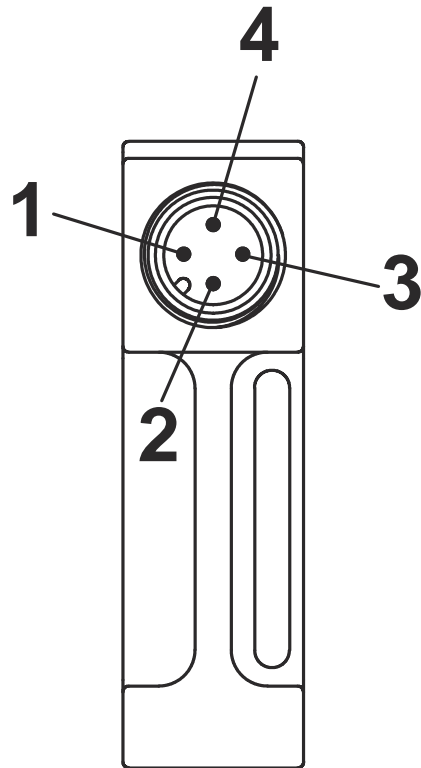


Fig. 16: Pin assignment, connector M12x1 (Form 15x50)

Wiring diagram

Normally Open (NOC):




Fig. 17: Switch position under no-flow condition

Change Over (COC):




Fig. 18: Switch position under no-flow condition

### 5.6.3 Switch contact SG-15 with cable

The individual cores of the cable are numbered according to the following connection diagram.

#### Wiring diagram

normally open:



Fig. 19: Switch position under no-flow condition

### 5.6.4 Degree of protection (IP-Code)

The specified degree of protection (IP) is only ensured if approved connection material is used (see following table).

Device connection	Specification of connection material	Degree of protection
EN1753 01-803 with gland	Diameter of connection cable: 5–6mm	IP65
M12x1	Plug connector M12x1	IP65
Cable	-	IP67

## 5.7 Grounding the device

When installing the device in a pipe system, ensure that the device is grounded to the pipe system to avoid a dangerous electrical potential difference.


## 5.8 Plug connection

### Personnel:

- Qualified electrician


### Tool:

- Flat-bladed screwdriver

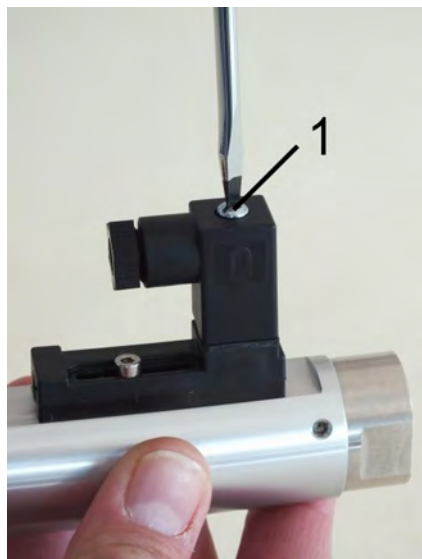


*Fig. 20: Detach socket*

1. ➔ Release the fixing screw (Fig. 20/1) from the socket

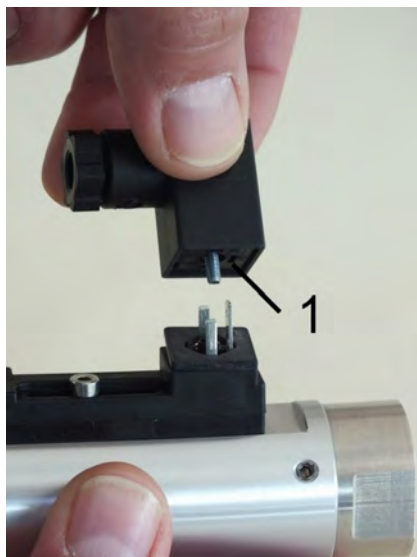

*Fig. 21: Remove socket*

2. ➔ Remove the socket (Fig. 21/1)

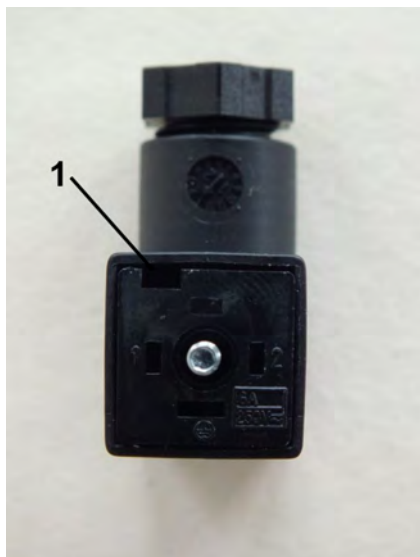

*Fig. 22: Loosen inner section*

3. ➤ Remove the plug insert from the plug by placing a flat-bladed screwdriver into the slot (Fig. 22/1) and carefully pry out the inner section.



*Fig. 23: Loosen the screw connection*

4. ➤ Unscrew the screw connection (Fig. 23/1) by turning it to the left
5. ➤ Guide the connecting cable through the screw connection into the female socket
6. ➤ Make the connections as shown in the connection diagrams (Fig. 24 und Fig. 25).
7. ➤ Position the plug insert (Fig. 22/1) back onto the plug and push until it locks.
8. ➤ Retighten the screw connection (Fig. 23/1) by turning it to the right

9. ➔ Plug the female socket onto the connector plug and tighten the fixing screw (Fig. 20/1).

Fig. 25: Pin assignment, plug socket, change-over contact (Form 15x50)

## 5.9 Contact protection measures

The Reed-switches used in the switch contacts are designed to be very sensitive to overload. To prevent destruction of the switch contact, the values specified on the rating plate of the switch contact must never be exceeded (not even temporarily).

There is a risk of overload from:

- inductive loads
- capacitive loads
- ohmic loads.

Suitable measures must be taken to protect against overload (see following examples):

### Inductive load

There is danger of voltage peaks from inductive loads when switching off (up to 10 times the rated voltage). Inductive loads are caused by, e.g.:

- Contactors, relays
- Solenoid valves
- Electric motors

Examples of protective measures:

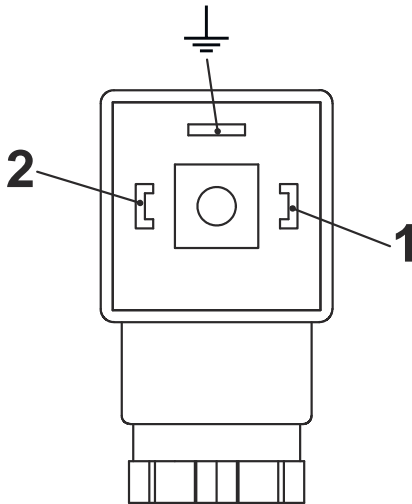
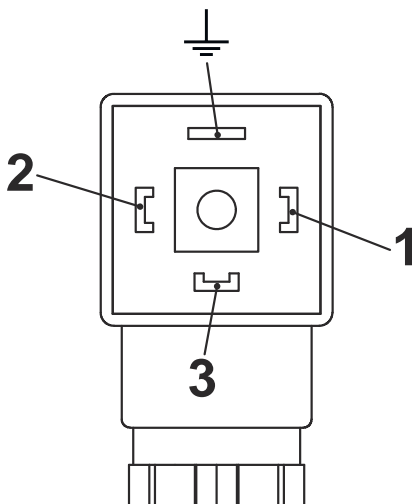


Fig. 24: Pin assignment, plug socket, normally-open contact (Form 15x50)





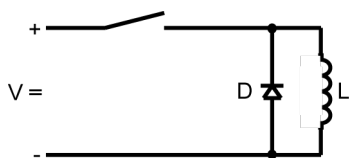


Fig. 26: Example 1

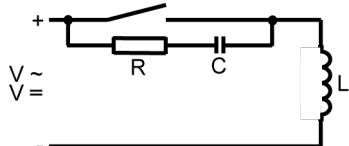


Fig. 27: Example 2

### Capacitive loads

There is a danger of high current peaks from capacitive loads when switching-on the switch contact (exceeding rated current). Capacitive loads are caused by, e.g.:

- Long connecting cables
- Capacitive consumers

Example of protective measure:

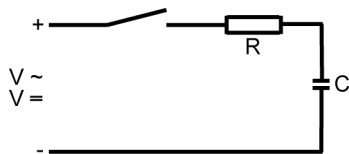


Fig. 28: Protective measure against capacitive loads

### Ohmic loads

There is a danger of high current peaks from ohmic loads when switching-on the switch contact. The reason for this is that the glow filament has a low resistance at low temperatures. Ohmic loads are caused by, e.g.:

- Filament bulbs
- Motors during startup

Examples of protective measures:

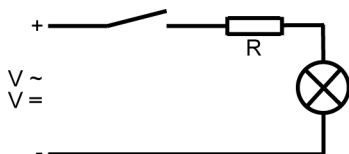


Fig. 29: Example 1

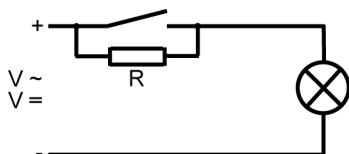


Fig. 30: Example 2

Protection against ohmic loads can be achieved through installation of a resistor in the circuit, or by heating the glow filament. For connection to high-impedance consumers (ex. PLC), a protective circuit is not needed.

## 6 Operation

### 6.1 Setting the switch point

#### Setting the switch point of an installed device



*The following instructions describe the procedure for a Normally Open Contact (NOC). The actual state (open or closed), can be determined using a continuity meter.*

**Personnel:**

- Qualified personnel

**Tool:**

- Hex screwdriver

1. Adjust the flow to be monitored and read it off at the scale on the device. The top edge of the float is the read-off point.



*Fig. 31: Loosen set screw*

2. Loosen the set screw of the switch contact (Fig. 31) using a hex screwdriver.
3. Slowly push the switch contact in the opposite direction of flow up to the stop.

### Condition 1: The contact is closed

4. ➤ Slowly push the switch contact in the direction of flow until the contact opens.

### Condition 2: The contact is open

5. ➤ Slowly push the switch contact in the direction of flow until the contact closes. Keep pushing slowly in the direction of flow until the contact opens.
6. ➤ Re-tighten the switch contact set screw (Fig. 31) using a hex screwdriver. When doing so, observe the correct tightening torque of the screw.

🔧 *Chapter 11.1 "Tightening torque" on page 76*

- ⇒ The set switch point corresponds to the switch-off point of the switch contact by decreasing flow.

### Setting the switch point of a non-installed device



Fig. 32: Loosen set screw

1. ➤ Loosen the set screw of the switch contact (Fig. 32) using a hex screwdriver.
2. ➤ Using a non-magnetic rod ( e.g. test rod), move the float to the point on the measuring scale that displays the flow rate to be monitored. The top edge of the float is the read-off point.
3. ➤ Slowly push the switch contact in the opposite direction of flow up to the stop.

### Condition 1: The contact is closed

4. ➤ Slowly push the switch contact in the direction of flow until the contact opens.

**Condition 2: The contact is open**

5. ➔ Slowly push the switch contact in the direction of flow until the contact closes. Then keep pushing slowly in the direction of flow until the contact opens.

6. ➔ Re-tighten the set screw of the switch contact (Fig. 32) using a hex screwdriver. When doing so, observe the correct tightening torque of the screw.

🔗 Chapter 11.1 "Tightening torque" on page 76

⇒ The set switch point corresponds the switch-off point of the switch contact by decreasing flow.

**6.2 Checking the flow****Reading-off the flow value****Personnel:**

- Qualified personnel

**Protective equipment:**

- Goggles

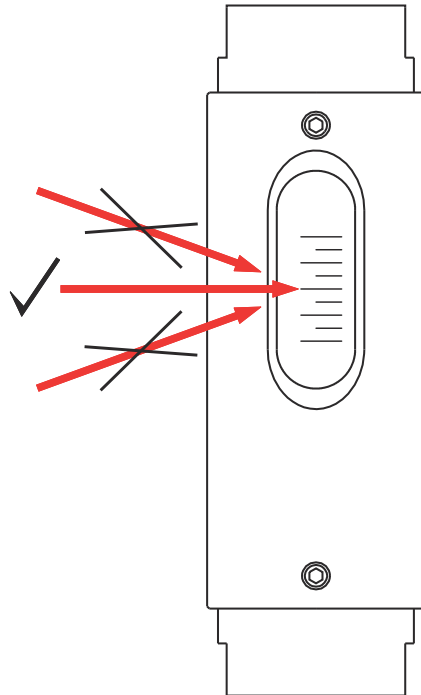




Fig. 33: Reading-off the measuring scale

1. ➔ The top edge of the float is the read-off point

2.  To obtain greatest reading accuracy, read-off at eye level. (Fig. 33, middle arrow). The read-off value can be falsified by viewing at an angle
3.  Read-off the flow value from the measuring scale

## 7 Troubleshooting

This chapter describes possible malfunctions of the device, their causes and repair.

If malfunctions persist or increase, shorten the maintenance interval to meet the actual operating conditions.

For malfunctions not described in this chapter, please contact the manufacturer (see service address on page 2).

### 7.1 Safety

**Work performed incorrectly to remedy a malfunction**



#### **WARNING!**

#### **Risk of injury due to incorrect repair of malfunction!**






Work performed incorrectly may result in severe injury and considerable damage to property

- Ensure that the site is sufficiently cleared before commencing work
- Ensure that the repair location is orderly and clean! Components and tools that are lying about or on top of each other are potential causes of accidents
- If components have been removed, observe correct assembly procedures. Reinstall all fixing/fastening elements and observe the prescribed tightening torque for the screws  
 ↪ *Chapter 11.1 "Tightening torque" on page 76*
- Before placing the device back into operation, ensure that all work has been performed and completed in compliance with the specifications and instructions in these Operating Instructions

### Conduct in case of malfunction

The complete machine or system may be unsafe if there is a defect at the flow monitor (e.g. broken sight glass).

The following always applies:

1.  In case of malfunctions that present an immediate danger to persons or valuables, proceed according to the valid emergency plans for the system
2.  Determine the cause of the malfunction
3.  Before repair, ensure that there is no danger to persons from escaping media
4.  If necessary, allow the pipeline and device to cool down or to warm up before commencing work
5.  Malfunctions must be corrected by qualified personnel



*The following troubleshooting guide provides an indication of who is qualified to repair the fault.*

## 7.2 Troubleshooting guide

Fault description	Cause	Remedy	Personnel
The switch contact does not switch.	No medium flowing through flow monitor	Check that medium is flowing through the pipe-line	Qualified personnel
	Flow is too low or the switch contact is set too high	<ul style="list-style-type: none"> <li>■ Adjust the switch contact to a lower flow rate</li> <li>■ Use the device at another measuring range</li> <li>■ Increase the flow rate</li> </ul>	Qualified personnel
	Incorrect reduction fitting or pipe diameter is too small	<ul style="list-style-type: none"> <li>■ Correct pipe diameter</li> </ul>	Qualified personnel
	Float is stuck	Disassemble and clean the device	Qualified personnel
	Switch contact is defective.	<ul style="list-style-type: none"> <li>■ Remedy the cause of the defect (short-circuit, overload)</li> <li>■ Replace the switch contact</li> </ul>	Qualified personnel
Switch contact is permanently switched.	Flow is too high or the switch contact is set too low	<ul style="list-style-type: none"> <li>■ Reduce the flow</li> <li>■ Adjust the switch contact to a higher flow rate</li> <li>■ Use the device at another measuring range</li> </ul>	Qualified personnel
	Float is stuck	Disassemble and clean the device	Qualified personnel



<b>Fault description</b>	<b>Cause</b>	<b>Remedy</b>	<b>Personnel</b>
Switch contact is permanently switched.	Switch contact is defective	<ul style="list-style-type: none"> <li>■ Remedy the cause of the defect (short-circuit, overload)</li> <li>■ Replace the switch contact</li> </ul>	Qualified personnel
The switch point is not the same as the actual flow rate.	Improper scale installed for media used	Request proper conversion table or scale for media used	Qualified personnel
	Incorrect reduction fitting or pipe diameter is too small	<ul style="list-style-type: none"> <li>■ Correct pipe diameter</li> </ul>	Qualified personnel
	Device is dirty	Disassemble and clean the device	Qualified personnel
	Device is defective	Remove device from system and contact the manufacturer	Qualified personnel

## 8 Maintenance

### 8.1 Safety

#### Maintenance work performed incorrectly



#### **WARNING!**

#### **Risk of injury due to maintenance work performed incorrectly!**

Maintenance work performed incorrectly can result in severe injury and considerable damage to property.

- Ensure that the site is sufficiently cleared before commencing work.
- Ensure that the repair location is orderly and clean! Components and tools that are lying about or on top of each other are potential causes for accidents.
- If components have been removed, observe correct assembly procedure. Reinstall all fixing/fastening elements and observe the prescribed tightening torque for the screws (see Chapter 11.1).

- Before placing the device back into operation ensure that all work has been performed and completed in compliance with the specifications and instructions in these Operating Instructions.

### 8.2 Maintenance plan

#### Intervals for replacing wear parts

RVO/U-L2 flow monitors require very little maintenance due to the small number of moving parts. The intervals for the replacement of wear parts depend significantly on the operating conditions as well as on the composition of the medium flowing through the device. For this reason, no intervals have been set by the manufacturer. The operator must determine suitable intervals based on the local conditions and circumstances.

Interval	Maintenance work	Personnel
	Visual inspection for dirt/soiling	Qualified personnel
	Visual inspection for free-movement of float	Qualified personnel
	Visual inspection for leaks from the device	Qualified personnel
	Check function of switch contact	Qualified personnel

## 8.3 Removal from the pipe system

The flow monitor must first be removed from the pipe system before performing maintenance work.



### **WARNING!**

#### **Risk of injury from pressurized lines!**

Severe injury may result if the pipe system is under pressure when removing the device.

- Depressurize the system before removing the device



### **WARNING!**

#### **Risk of injury from hot or cold surfaces!**

Pipelines can heat up/cool down dramatically due to the media flowing through them. Skin contact with hot or cold surfaces causes severe skin burn or frostbite.

- Before removing the device, ensure that the machine or system and the flow monitor have been controlled to a temperature range between 0 °C and 40 °C
- Do not touch any part of the machine or system that is either very cold or very hot
- Always wear heat-resistant/cold-resistant protective work clothing and protective gloves when working near hot/cold surfaces

**WARNING!****Risk of injury from media in the pipe system!**

If the pipe system contains toxic or hazardous media, severe injury may be caused by escaping media!

- Before removing the device, ensure that the pipe system is empty and does not contain any media residue
- Always wear personal protective equipment when removing the device

**WARNING!****Risk of injury from media residue in the device!**

After the pipe system has been emptied, media residue can still be present inside the device. In the case of toxic or hazardous media, this could result in serious injury.

- When removing (deinstalling the device from the pipe system), always wear personal protective equipment.
- All requirements specified in the media safety data sheet must be observed in accomplishing the work task.
- Residue of toxic or hazardous media in the device can result in serious injury.

## Removing the device from the pipe system

### Personnel:

- Qualified personnel

### Protective equipment:

- As specified in the Safety Data Sheet of the medium, protective equipment must be worn when handling hazardous media. In addition, the specifications of the system operator must be followed. If no protective equipment is specified, suitable protective gloves and goggles must be worn.

### Tool:

- Fixed spanner

1. ▶ Loosen the adapter union of the pipeline using a suitable spanner. When doing so, lock the process connection in place with a second spanner.
2. ▶ Secure the device against falling and repeat Step 1 at the other end of the device

## 8.4 Disassembly

To replace wear parts or to clean the device, the flow monitor must first be disassembled.



### WARNING!

#### Risk of injury due to incorrect disassembly!

- The device may still contain media residue
- Wear personal protective equipment when working with dangerous media
- Improper disassembly may cause serious injuries if dangerous media is still present inside the device



### CAUTION!

#### Risk of injury due to incorrect disassembly!

Incorrect disassembly may result in injuries.

- Before disassembling, ensure that the flow monitor has cooled down/ warmed up to a temperature range between 0 and 40° C
- Wear personal protection equipment to protect against hazardous media which may still be present inside the device.

**Protective equipment:**

- As specified in the Safety Data Sheet of the medium, protective equipment must be worn when handling hazardous media. In addition, the specifications of the system operator must be followed. If no protective equipment is specified, suitable protective gloves and goggles must be worn.

**Personnel:**


- Qualified personnel

**Protective equipment:**

- Goggles
- Protective gloves

**Tool:**

- Hex screwdriver

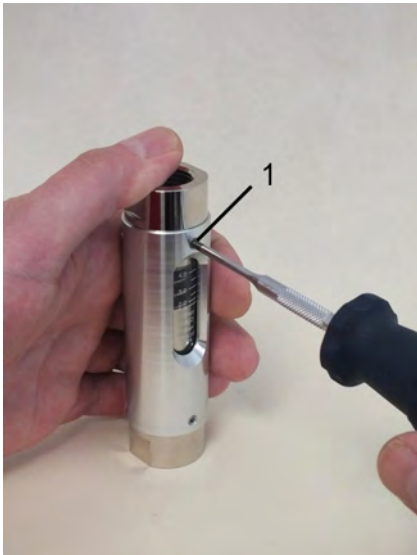*Fig. 34: Loosen screws*

1. ➤ Loosen the top 3 hex head screws (Fig. 34/1) using a hex screwdriver.

*Fig. 35: Remove the process connection (outlet)*

2. ➤

**CAUTION!**

Carefully pull the process connection (outlet) from the device body, turning slightly when doing so (Fig. 35). Do not apply undue force.

The sight glass can break if too much force is exerted or if the process connection is canted.

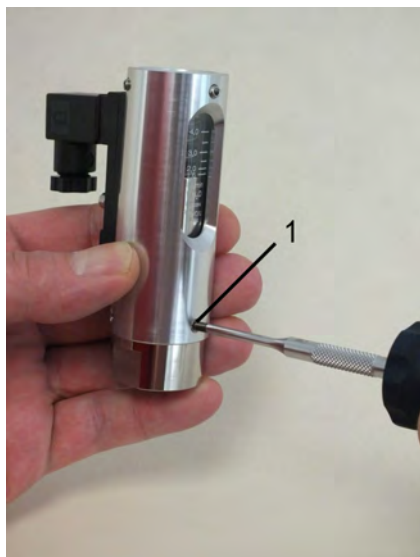


Fig. 36: Loosen screws

3. ➤ Secure the device with one hand to ensure the sight glass does not slip out, then loosen the lower 3 hex head screws (Fig. 36/1).



Fig. 37: Remove the inner parts

4. ➤ Carefully remove the inner parts (Fig. 37/1) of the device (sight glass, spring and float) as a unit together with the process connection (inlet) (Fig. 37/2) from the device body



Fig. 38: Remove float and spring

5. ➤ Rotate the inner section 180° and remove the spring and float
6. ➤ Remove the sight glass from the process connection (inlet) by twisting lightly.
7. ➤ If necessary, remove the O-rings from the individual parts



#### **O-ring replacement**

*It is recommended that the O-rings be replaced during maintenance.*

## 8.5.1 Cleaning

It is the responsibility of the operator to establish appropriate intervals and procedures for cleaning the individual parts of the device. It must be ensured that the parts are not damaged during the cleaning process. When using cleaning agents, it must be ensured that these are not aggressive to the parts and that there will be no dangerous reactions with media residue. Damaged parts must be replaced.



### **WARNING!**

#### **Risk of injury due to improper cleaning!**

The device may still contain media residue.

- To protect against hazardous media residue in the device, wear personal protective equipment.
- Do not use cleaning agents that cause dangerous reactions with media residue.
- All requirements specified in the Safety Data Sheet must be observed when handling or otherwise using this medium
- Residue of hazardous media inside the device can cause serious injury.

## 8.5 Maintenance





### CAUTION!

#### Risk of injury due to damaged parts!

If parts of the device are broken or damaged, they may cause injury due to sharp edges or splinters during the cleaning process.

- Damaged parts must be replaced
- Carefully clean the parts of the device, so as not to cause damage, this is especially so for the sight glass
- When cleaning, always wear appropriate personal protective equipment
- Incorrect disassembly can result in injuries

#### Protective equipment:

- As specified in the Safety Data Sheet of the medium, protective equipment must be worn when handling hazardous media. In addition, the specifications of the system operator must be followed. If no protective equipment is specified, suitable protective gloves and goggles must be worn.

## 8.5.2 Parts replacement

Depending on the operating conditions, wear parts such as O-rings, float and sight glass may have to be replaced. Steps required to replace these parts correspond to those used when assembling the device  
 ↪ *Chapter 8.5.3 "Assembly" on page 57.*

## 8.5.3 Assembly

The flow monitor must be reassembled after cleaning the individual components.

**Personnel:**

- Qualified personnel

**Tool:**

- Hex screwdriver
- Torque screwdriver and assorted blades

**Special Tools:**

- Test rod



Fig. 39: O-ring (seal)

1. ➤ Carefully install the O-ring (seal) onto the process connection (Fig. 39/1), so that it rests in the upper O-ring groove of the process connection (Fig. 41). When doing so, be careful not to overstretch the O-ring.



Fig. 40: O-ring (glass buffer)

2. ➤ Carefully seat the O-ring (glass buffer) on the process connection (Fig. 40/1), so that it is properly seated on the lower portion of the process connection (Fig. 41). When doing so, be careful not to overstretch the O-ring.

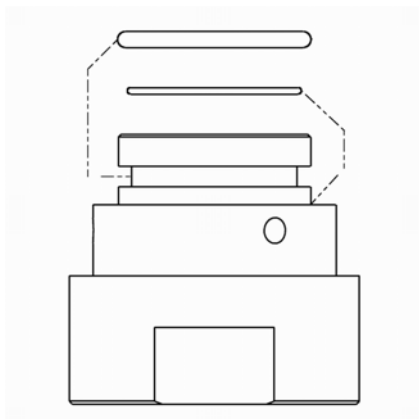


Fig. 41: Position of O-rings

3. ➔ Repeat steps 1 and 2 for the second process connection.



Fig. 42: Inner parts

4. ➔ Insert the spring (Fig. 42) into the float.

5. ➔ Lubricate the process connection O-rings lightly.



A list of suitable lubricants is contained in the annex & Chapter 11.5 "Lubricants" on page 79.



Fig. 43: Process connection (inlet) and sight glass

6. **CAUTION!**

Carefully insert the process connection (inlet) (Fig. 43/1) into the sight glass, pressing lightly

The sight glass can break if too much force is exerted or if the process connection is canted.

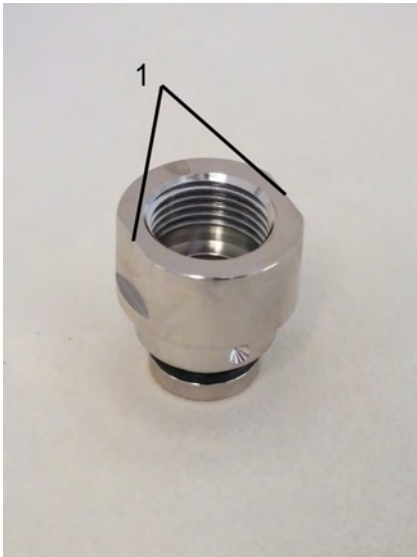


Fig. 44: Spanner flats

7. 


Position the process connection (inlet) so that the spanner flats (Fig. 44/1) are at a 90° angle to the sight glass scale. The locating pin hole on the process connection must be centered on the front of the device housing locating screw.



Fig. 45: Insert process connection into device housing

8. 

Insert the process connection (inlet) along with the sight glass into the device housing (Fig. 45) and axially align the connection to the housing. The locating pin hole in the process connection must be centered to the front locking screw of the device housing.

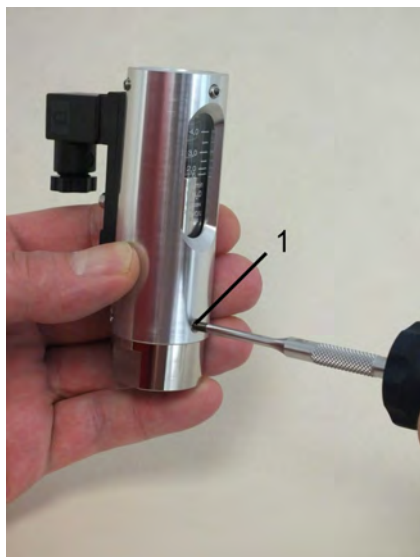

*Fig. 46: Secure the process connection (inlet)*

9. ➤ Secure the process connection (inlet) with 3 hex socket screws (Fig. 46/1) to the device housing, observing the proper torque ➤ Chapter 11.1 "Tightening torque" on page 76



*Fig. 47: Center the sight glass*

10. ➤ Center the sight glass scale on the window of the device housing.



*Fig. 48: Insert the inner parts*

- 11.** ➤ Insert the float and spring into the device housing



*Fig. 49: Position the process connection (outlet)*

- 12.** ➤ Insert the process connection (outlet) into the device housing
- 13.** ➤ Insert the outlet process connection (Fig. 49) into the device housing, turning lightly. (Fig. 49) When doing so, ensure that the spanner flats are at an angle of 90 ° to the sight window of the device housing.

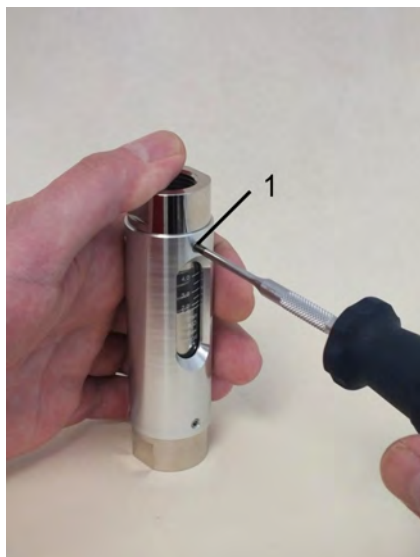


Fig. 50: Tighten hex socket screws

14. ▶ Tighten the 3 hex socket screws (Fig. 50/1), observing the proper torque ( ↗ Chapter 11.1 “Tightening torque” on page 76).



Fig. 51: Check for free movement

15. ▶ Check the float for ease of movement by applying light pressure with the test rod (Fig. 51).
  - ⇒ If the float moves sluggishly then disassemble the device ( ↗ Chapter 9.2 “Disassembly” on page 67) and clean the float and sight glass.




*If the float is still sluggish after having been cleaned several times, contact the manufacturer.*

## 8.5.4 Switch contact replacement


### Tool:

- Flat-bladed screwdriver
- Hex screwdriver

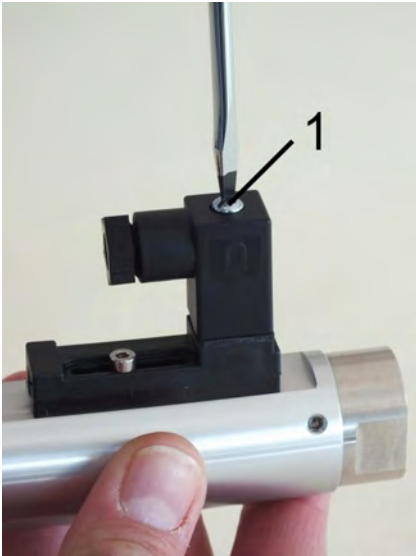

*Fig. 52: Loosen female socket*

1. ➔ Loosen the fixing screw (Fig. 52/1) of the female socket with a flat-bladed screwdriver.

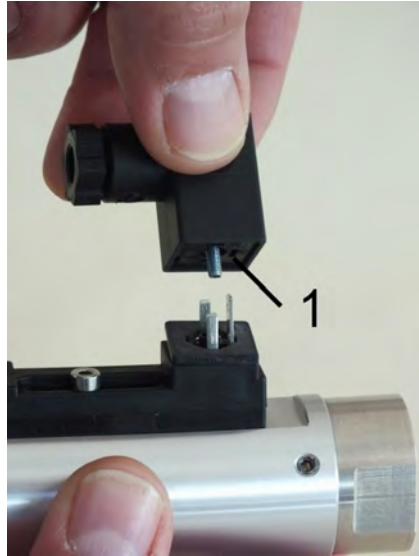

*Fig. 53: Remove the female socket*

2. ➔ Remove the female socket and gasket (Fig. 53/1) by pulling upwards





*Fig. 54: Remove set screw*

3. ➤ Using a hex screwdriver (Fig. 54/1) remove the set screw of the switch contact



*Fig. 55: Remove switch contact*

4. ➤ Remove the switch contact from the guide surface (Fig. 55)
5. ➤ Attach the new switch contact
6. ➤ The guide groove of the switch contact must be slipped over the cylinder pin
7. ➤ Insert the set screw (Fig. 54/1) and tighten it slightly so that the switch contact can still move easily
8. ➤ Adjust the required switch point by moving the switch contact to the desired position
9. ➤ Retighten the set screw (Fig. 54/1), observing the proper tightening torque ( ↗ Chapter 11.1 "Tightening torque" on page 76)

10. ➤ Position the female socket and gasket, then tighten the fixing screw.

## 8.6 Measures to be taken after maintenance work

Take the following steps after completion of maintenance work and before switching on the device:

1. ➤ Check all previously loosened/ released screw connections for tightness.  
*🔗 Chapter 11.1 "Tightening torque" on page 76*
2. ➤ Clean the work area and remove all residual materials, packaging, substances or spills.

## 9 Disassembly and disposal

After its period of useful life, the device must be disassembled and disposed of in an environmentally safe manner.

### 9.1 Safety



#### **WARNING!**

#### **Risk of injury if disassembled incorrectly!**

Media residue, sharp edged components, pointed ends and corners on and in the device or on tools may cause injury.

- Ensure that the site is sufficiently cleared before commencing work
- Always wear protective equipment when handling hazardous media residue
- Handle open, or sharp-edged components carefully
- Ensure that the workplace is orderly and clean! Components and tools that are lying about or on top of each other are potential causes for accidents
- Disassemble components professionally
- Secure components so that they do not fall or overturn
- If in doubt, contact the manufacturer

### 9.2 Disassembly

Before starting disassembly:



- Remove operating materials and packaging and dispose of properly.

#### **Personnel:**

- Qualified personnel

#### **Protective equipment:**

- Protective gloves
- Goggles

1. ➤ Remove the device from the pipeline (  *Chapter 8.3 "Removal from the pipe system" on page 51*)
2. ➤ Disassemble the device (  *Chapter 8.4 "Disassembly" on page 53*)
3. ➤ Clean components properly
4. ➤ Dispose properly

### 9.3 Return Materials

#### 9.3.1 Return Materials Authorization

For products being returned, regardless of the reason, the currently valid provisions of the returns policy set by MEISTER will apply. Return shipments which do not comply with the returns policy may be refused by MEISTER at the expense of the consignor.

## 9.4 Disposal

If no return or disposal agreement has been made, recycle disassembled components:

- Scrap metals
- Recycle plastic elements
- Dispose of the remaining components according to their material properties

### **! NOTICE!**

#### **Danger to the environment due to incorrect disposal!**

Potential risk to the environment may arise due to incorrect disposal.

- Have electrical scrap, electronic components, lubricants and other supplies disposed of by approved specialists
- In case of doubt, obtain information on environmentally safe disposal from the local authority or special disposal expert

## 10 Technical data

### 10.1 Device data plate

The data plate is on the mechanical part of the flow monitor/flowmeter and contains the following information:



Fig. 56: Device data plate

### 10.2 Switch contact rating plate




Fig. 57: Switch contact rating plate





Fig. 58: Switch contact rating plate with positioning arrow

The rating plate is on the switch contact and may provide the following information:

- maximum voltage
- maximum current
- maximum power
- positioning arrow for cut-off point

## 10.3 Dimension sheet

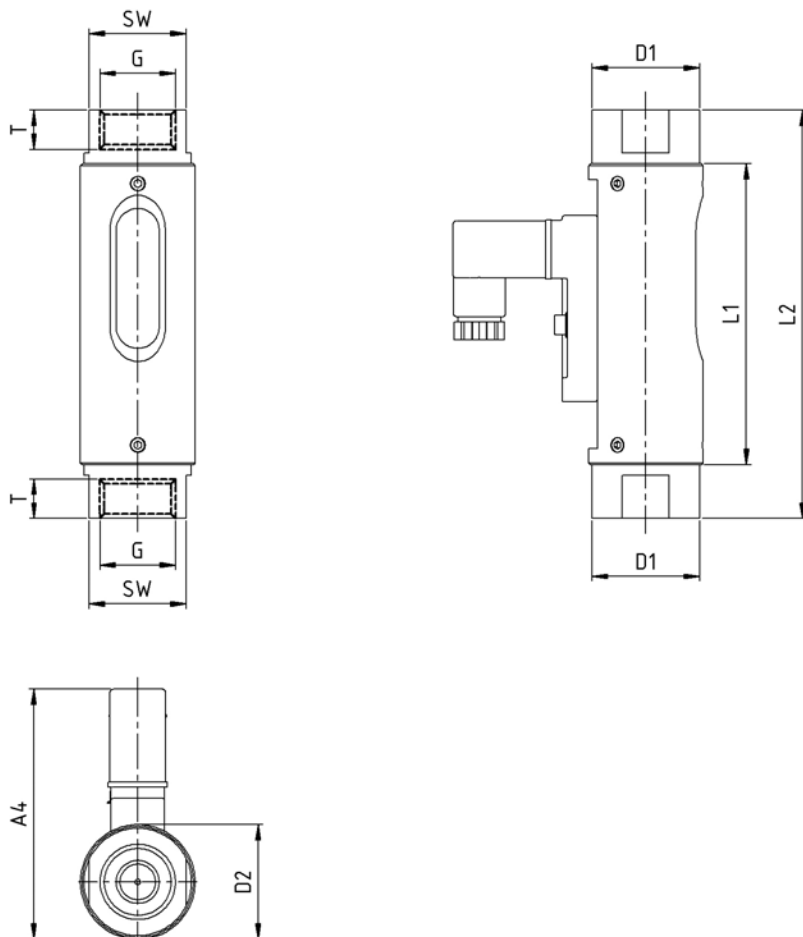

## 10.4 General specifications

Type	Overall dimensions (mm)					
	G	DN	SW	L1	L2	T
RVO/U-L20012	1/2"	15	27	84	114	14
RVO/U-L20030	1/2"	15	27	84	114	14
RVO/U-L20040	1/2"	15	27	84	114	14
RVO/U-L20080	1/2"	15	27	84	114	14
RVO/U-L20125	1/2"	15	27	84	114	14
RVO/U-L20200	1/2"	15	27	84	114	14
RVO/U-L20420	1/2"	15	27	84	114	14
RVO/U-L20500	1/2"	15	27	84	114	14

Type	Overall dimensions (mm)							Weight (g)
	G	D1	D2	A1	A2	A3	A4	
RVO/U-L20012	1/2"	30	32	-	-	-	70	300
RVO/U-L20030	1/2"	30	32	-	-	-	70	300
RVO/U-L20040	1/2"	30	32	-	-	-	70	300

Type	Overall dimensions (mm)							
	G	D1	D2	A1	A2	A3	A4	Weight (g)
RVO/U-L20080	1/2"	30	32	-	-	-	70	300
RVO/U-L20125	1/2"	30	32	-	-	-	70	300
RVO/U-L20200	1/2"	30	32	-	-	-	70	300
RVO/U-L20420	1/2"	30	32	-	-	-	70	300
RVO/U-L20500	1/2"	30	32	-	-	-	70	300



*NPT threads are available on request.*

*The weight of the connection cable at a length of 2m is approx. 80 g.*

## 10.5 Electrical specifications

### Change-Over Contact (COC)

Data	Value	Unit
Voltage	250	V
Current, maximum	1,5	A
Power, maximum	50	VA
Minimum load	3	VA



**Normally Open Contact (NOC)**

<b>Data</b>	<b>Value</b>	<b>Unit</b>
Voltage	230	V
Current, maximum	3	A
Power, maximum	60	VA

**Change-Over Contact (COC) M12x1 (-20 °C–85 °C)**

<b>Data</b>	<b>Value</b>	<b>Unit</b>
Voltage	125	V
Current, maximum	1,5	A
Power, maximum	50	VA
Minimum load	3	VA

**Normally Open Contact (NOC) M12x1 (-20 °C–85 °C)**

<b>Data</b>	<b>Value</b>	<b>Unit</b>
Voltage	125	V
Current, maximum	3	A
Power, maximum	60	VA

## Change-Over Contact (COC) SPS

Data	Value	Unit
Voltage	250	V
Current, maximum	1	A
Power, maximum	60	VA

## 10.6 Measuring ranges

### 10.6.1 Standard measuring ranges

Type	Switch range for air at 1 bar abs. & 20 °C		
	NI/min	SCFH	SCFM
RVO/U-L20012	3 – 12	6,5 – 25,0	–
RVO/U-L20030	7 – 30	15,0 – 64,0	–
RVO/U-L20040	12 – 40	25,0 – 85,0	–
RVO/U-L20080	20 – 80	–	0,7 – 2,8
RVO/U-L20125	28 – 125	–	1,0 – 4,4
RVO/U-L20200	50 – 200	–	1,8 – 7,0
RVO/U-L20420	100 – 420	–	3,5 – 14,8
RVO/U-L20500	200 – 500	–	7,1 – 17,7



*The specified data are switch-off points. Other switch ranges are available on request.*

## 10.7 Operating data

Description	Value	Unit
Max media temp.	100 (optional: 160)	°C
Min media temp.	-20	°C
Max. operating pressure	16	bar
Pressure loss	0,02 – 0,3	bar
Measuring accuracy	± 10 % of full scale value	

### **! NOTICE!**

It must be ensured that the medium does not freeze.

Operating data for devices employed in explosion hazard zones differs from the above and are specified in the Operating Instructions for "RVO/U-L2 Module ATEX, Chapter 4.


# 11 Annex

## 11.1 Tightening torque

Component/ function	Description	Size	Torque	Number
Device housing screw	Hexagon socket screw	M4x5	1,4 Nm	6
Switch contact housing assembly screw	Cylinder head screw	M3x10	0,4 Nm	1

## 11.2 Replacement parts

The following replacement parts drawing provides an example of the construction of an RVO/U-L2 type flow monitor. The actual configuration may vary depending on the model.

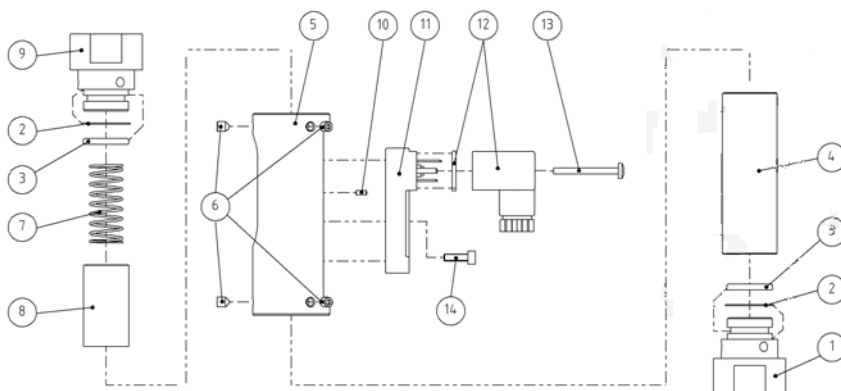

Item	Qty	Description
1	1	Process connection (inlet)
2	2	O-Ring (glass buffer)
3	2	O-Ring (seal)
4	1	Sight glass
5	1	Device housing
6	6	Hex socket screw
7	1	Spring
8	1	Float
9	1	Process connection (outlet)
10	1	Cylinder pin (switch contact)

Item	Qty	Description
11	1	Switch contact with male connector
12	1	Female socket and gasket
13	1	Fixing screw (female socket)
14	1	Set screw (switch contact)

## 11.3 Tools

The following tools are required:

### Tools

- Fixed spanner 27 mm
- Flat-bladed screwdriver, blade width 5,5mm
- Hex screwdriver 2 mm
- Hex screwdriver 2,5 mm
- Torque screwdriver, and assorted blades

### Special tool

- Test rod RVO/U-L2

## 11.4 Sealant



*Before using a sealant, ensure that it is compatible with the media used and that it can be employed under the given operating conditions.*

- Ensure proper seal
- Use a suitable sealant. Liquid sealants will damage the flow monitor
- Always follow the sealant manufacturer's instructions

## 11.5 Lubricants



*Before using a lubricant, always make sure that it is compatible with the operating medium.*

For the proper mounting of O-rings, device-specific O-ring installation tools may be purchased from the manufacturer.

The following lubricants are suitable to facilitate installing the O-rings:

Lubricant	O-ring material		
	NBR	EPDM	FKM
Glycerine*	suitable	suitable	suitable
Soapy water	suitable	suitable	suitable

\* Glycerine must not be used if the device is used for sulfuric acid and/or nitric acid.

## 12 Index

### A

Application . . . . .	10
Assembly . . . . .	57

### C

Cable . . . . .	37
Component groups . . . . .	21
Connected loads	
NOC . . . . .	73
Connector	
M12x1 . . . . .	36
Contact . . . . .	7
Contact protection measures . . . . .	40
Copyright . . . . .	3
Correct use in accordance with these instructions . . . . .	10
Customer service . . . . .	7

### D

Degree of protection	
IP-Code . . . . .	37
Device data plate . . . . .	69
Device description . . . . .	20
Dimension sheet . . . . .	70
Disassembly	
maintenance . . . . .	53
Disassembly	
Disposal . . . . .	67
Disposal . . . . .	68

### E

Electrical connection . . . . .	34
Environmental protection . . . . .	17
cleaning fluids . . . . .	17
lubricants . . . . .	18

### F

Fault table . . . . .	48
-----------------------	----

### G

General	
safety . . . . .	8

### H

Hazard	
electrical current . . . . .	12
Hazards	
mechanical . . . . .	12
media . . . . .	14
radiation . . . . .	14
temperature . . . . .	13

### I

Initial startup . . . . .	33
Installation	
pipe system . . . . .	30
preparations . . . . .	27

### L

Limitation of liability . . . . .	3
Lubricant . . . . .	79



## M

Maintenance . . . . .	56
Maintenance plan . . . . .	51
Measuring range . . . . .	74

## O

Operating conditions . . . . .	75
Overview . . . . .	20
Owner . . . . .	18

## P

Packaging . . . . .	22
Parts replacement . . . . .	57
Plug connection . . . . .	38
Plug connector	
EN175301-803 . . . . .	35
Precautions	
general . . . . .	11
Preparation	
Device . . . . .	30

## R

Read-off	
flow value . . . . .	44
Replacement parts . . . . .	17, 77
Return Materials Authorization . . . . .	67

## S

Safety	
disassembly . . . . .	67
Safety equipment . . . . .	15, 16

## Safety instructions

transport . . . . .	22
---------------------	----

Sealant . . . . .	78
-------------------	----

Service . . . . .	7
-------------------	---

Sight glass . . . . .	21
-----------------------	----

## Specifications

Change-Over Contact (COC) . . . . .	72
-------------------------------------	----

Storage . . . . .	23
-------------------	----

Strainer . . . . .	29
--------------------	----

Switch contact . . . . .	21
--------------------------	----

replacement . . . . .	64
-----------------------	----

Switch contact rating plate . . . . .	69
---------------------------------------	----

Switch point adjustment . . . . .	42
-----------------------------------	----

## Symbols

packaging . . . . .	23
---------------------	----

## Symbols used

in the instructions . . . . .	8
-------------------------------	---

## T

### Technical data

General specifications . . . . .	71
----------------------------------	----

Tightening torque . . . . .	76
-----------------------------	----

Tightening torque of screws . . . . .	76
---------------------------------------	----

Tools . . . . .	78
-----------------	----

Transport inspection . . . . .	22
--------------------------------	----

## U

Unimpeded flow sections . . . . .	28
-----------------------------------	----

## W

Warranty and guarantee provisions . . . . .	7
---	---